

# Medical Device Change ALERT

## IV Start Kit



**IMPORTANT**




**251125**



# General Overview -

# Current Device


# General Overview - Existing

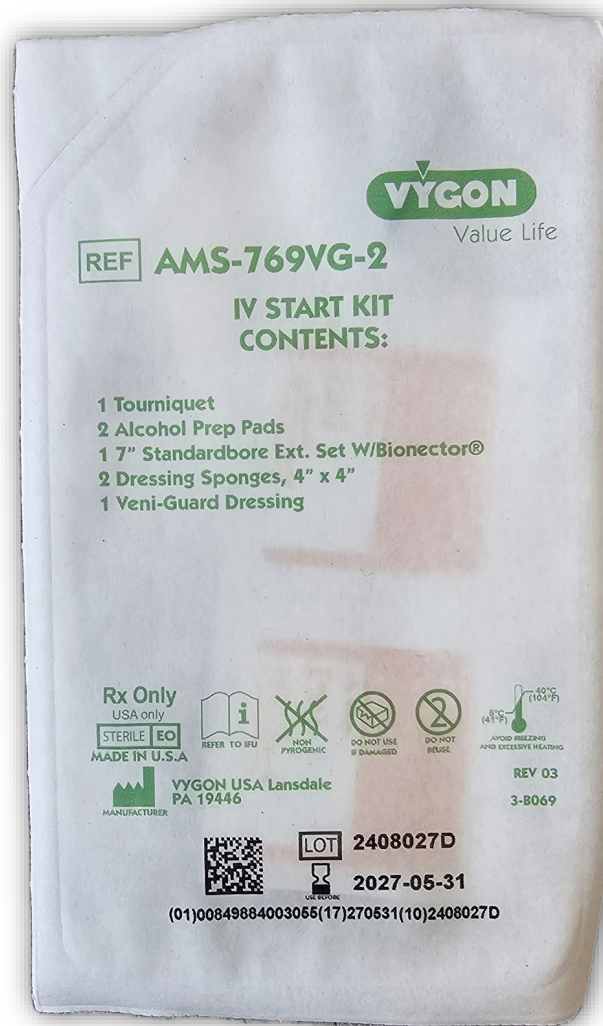

# General Overview - Current (cont.)



# General Overview - Current (cont.)

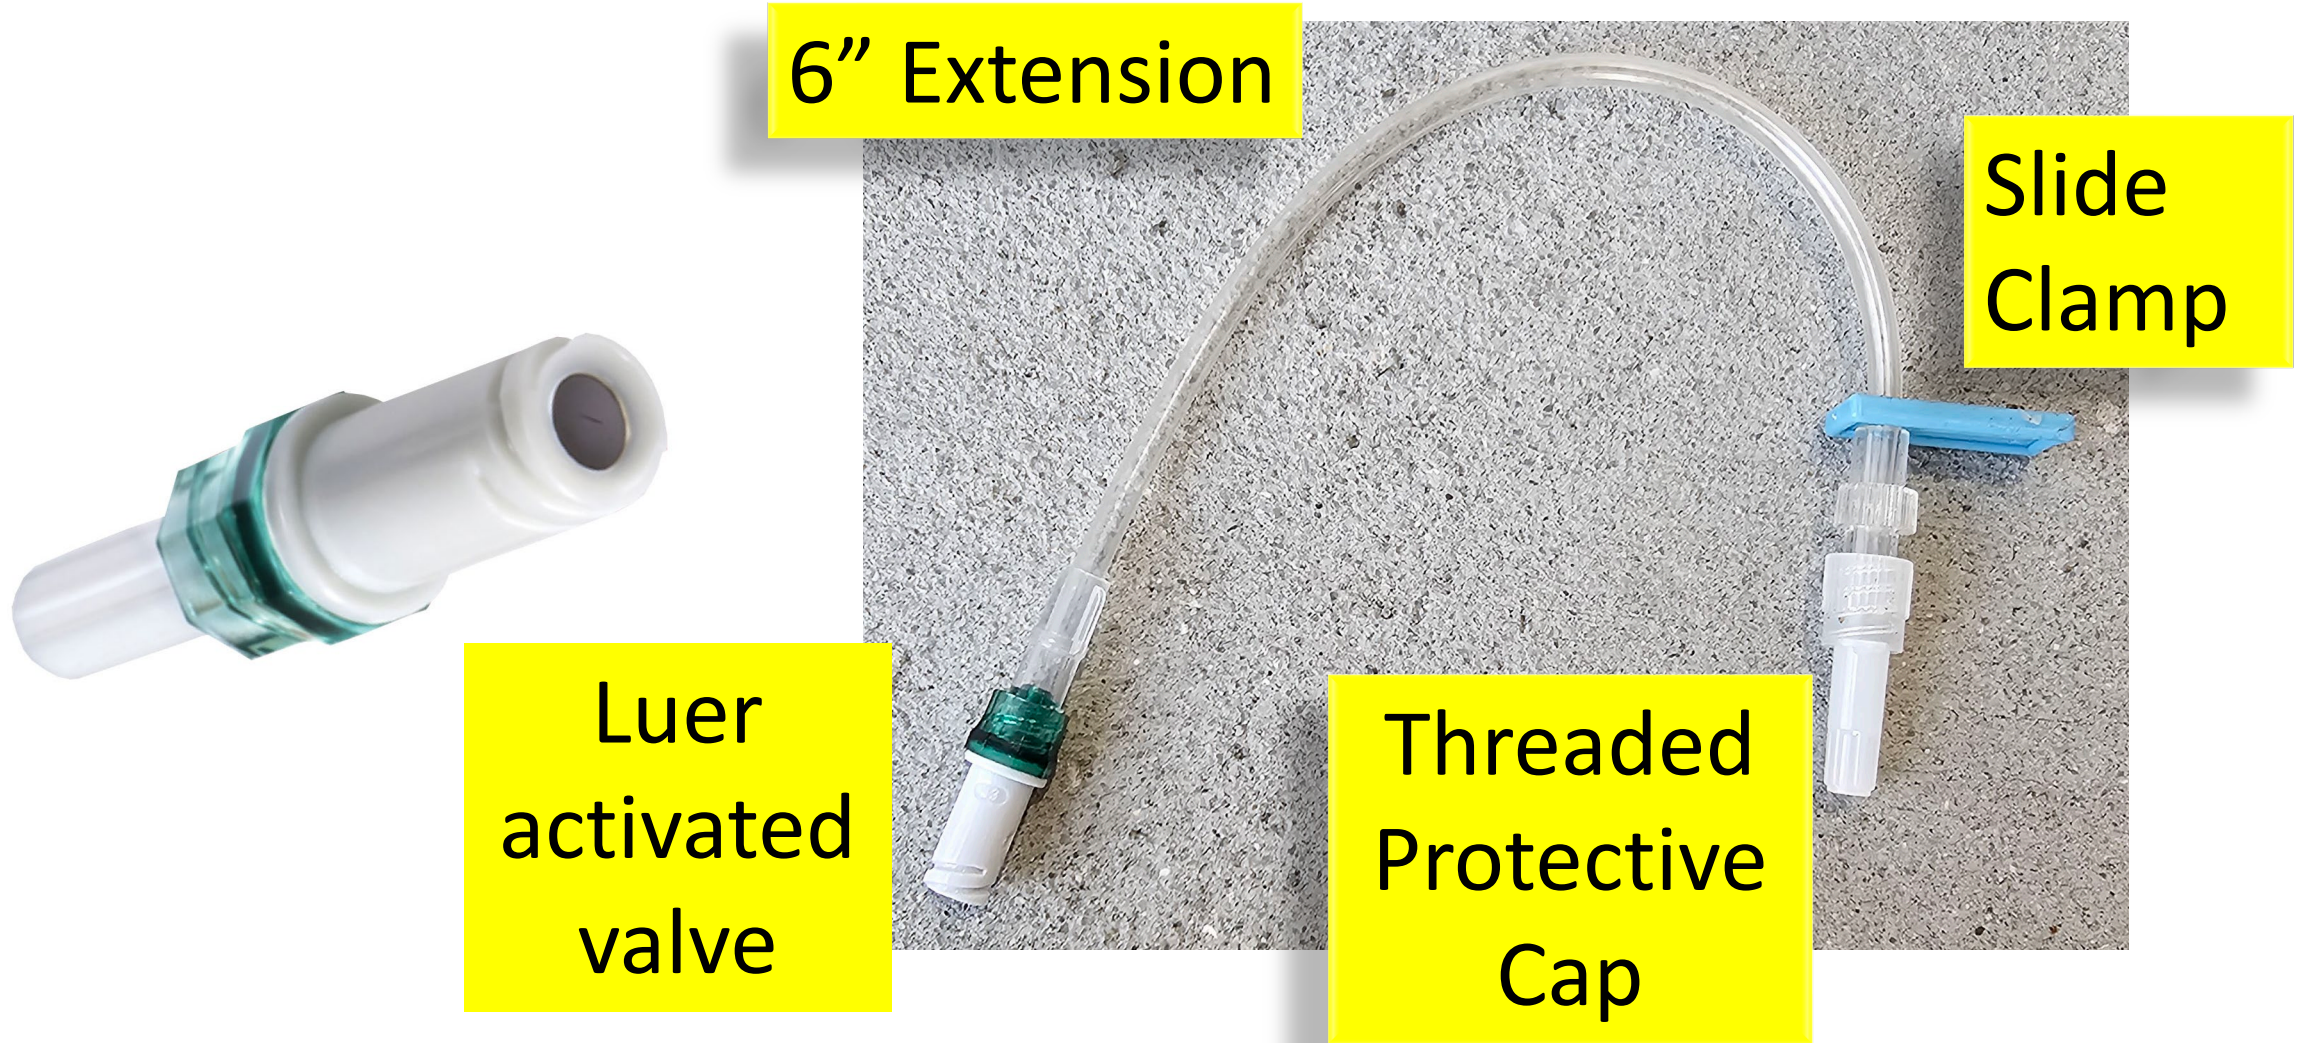



# NEW

# - General Overview




**NEW**

# - General Overview



# **NEW** - General Overview

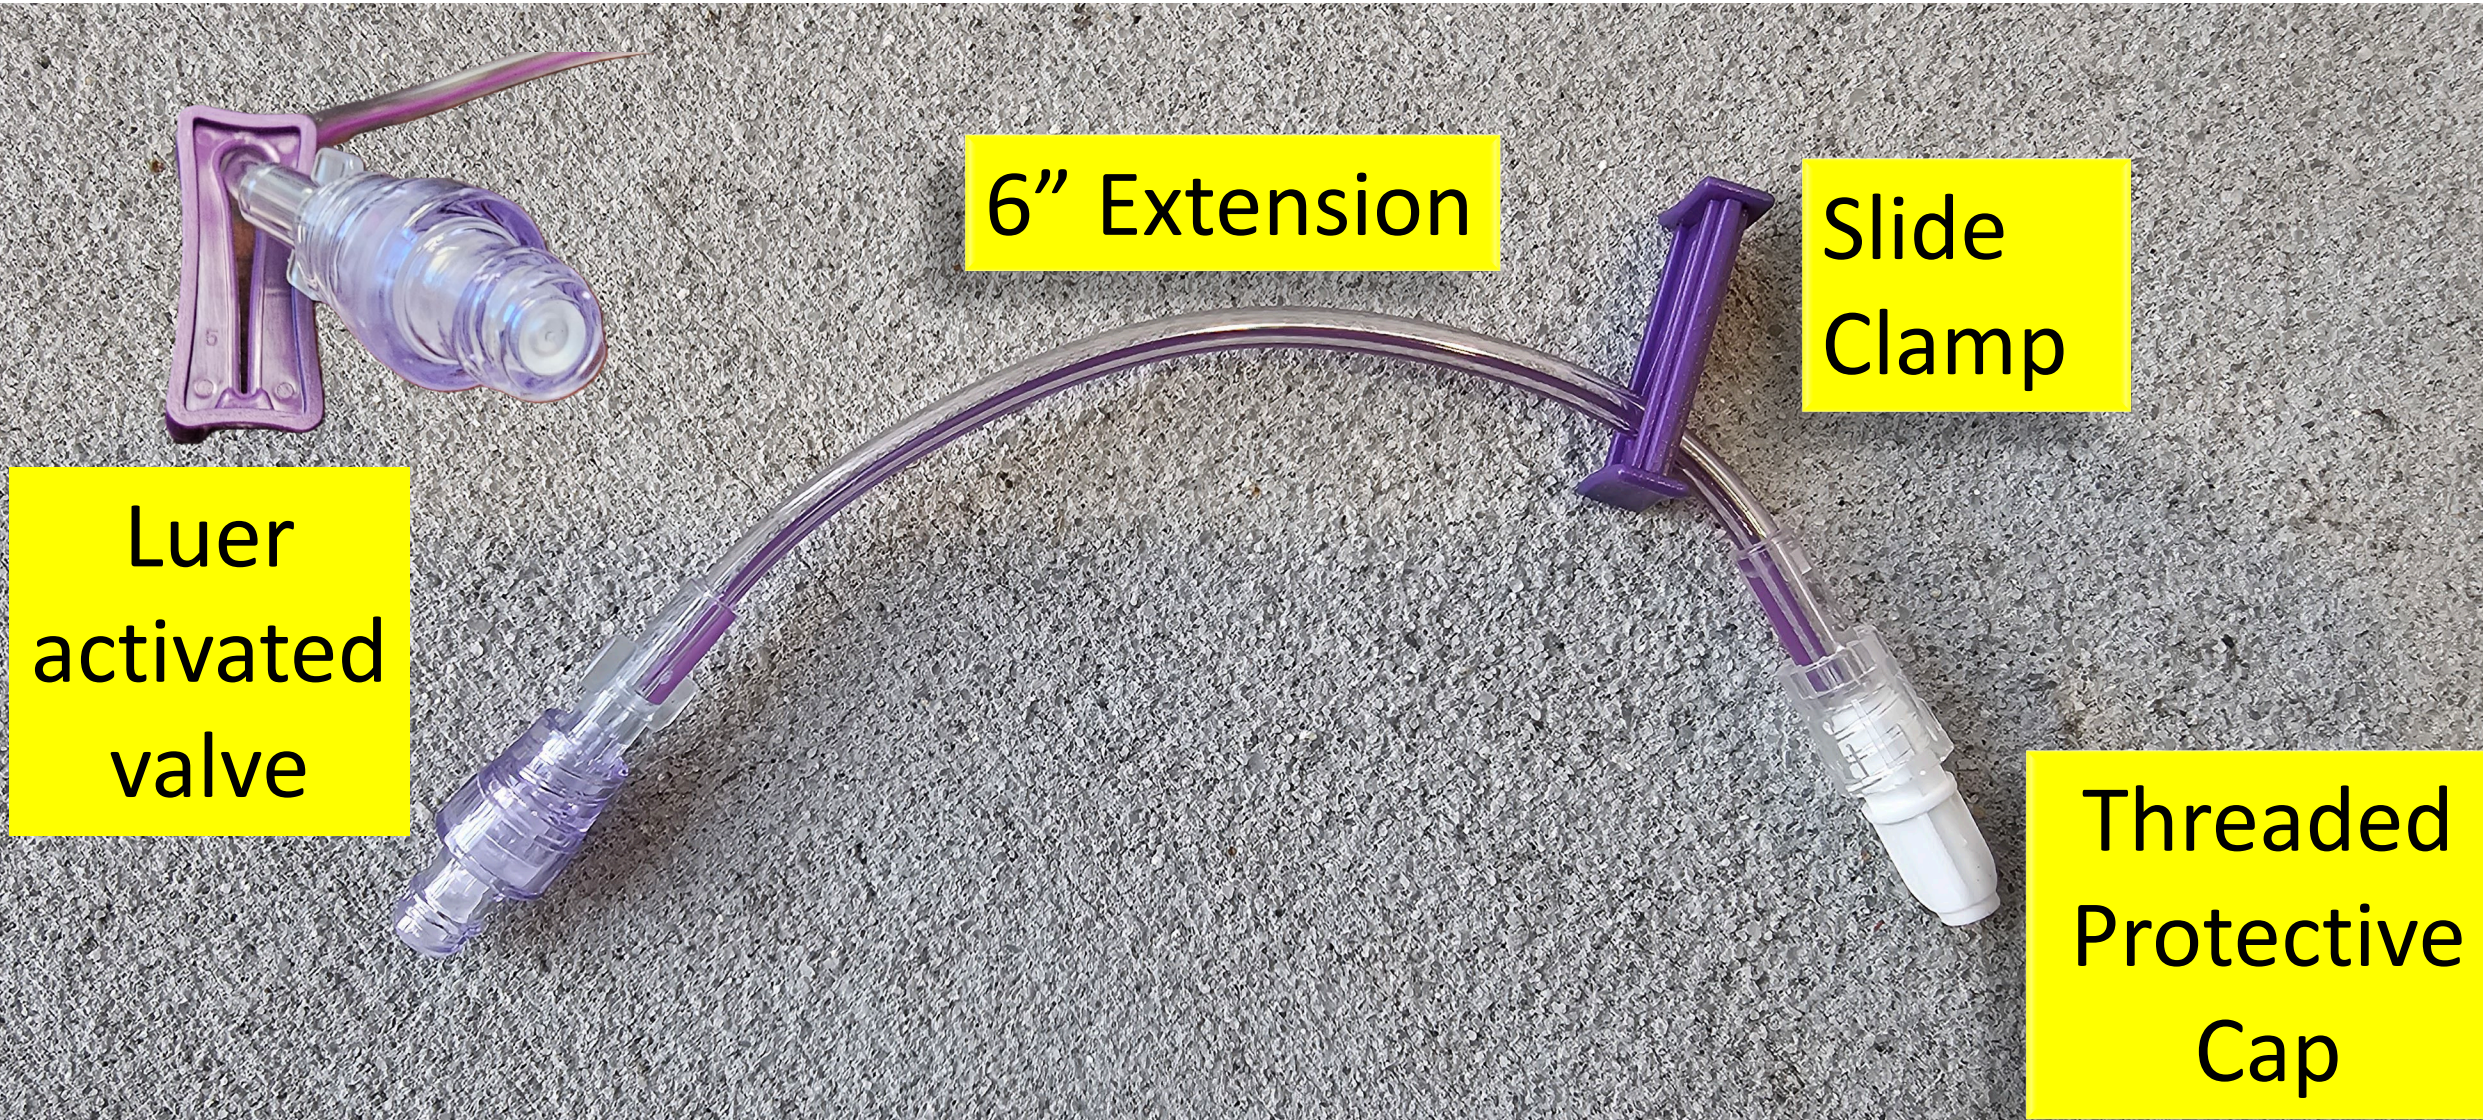


Luer  
activated  
valve

6" Extension

Slide  
Clamp

Threaded  
Protective  
Cap

# **NEW** - General Overview

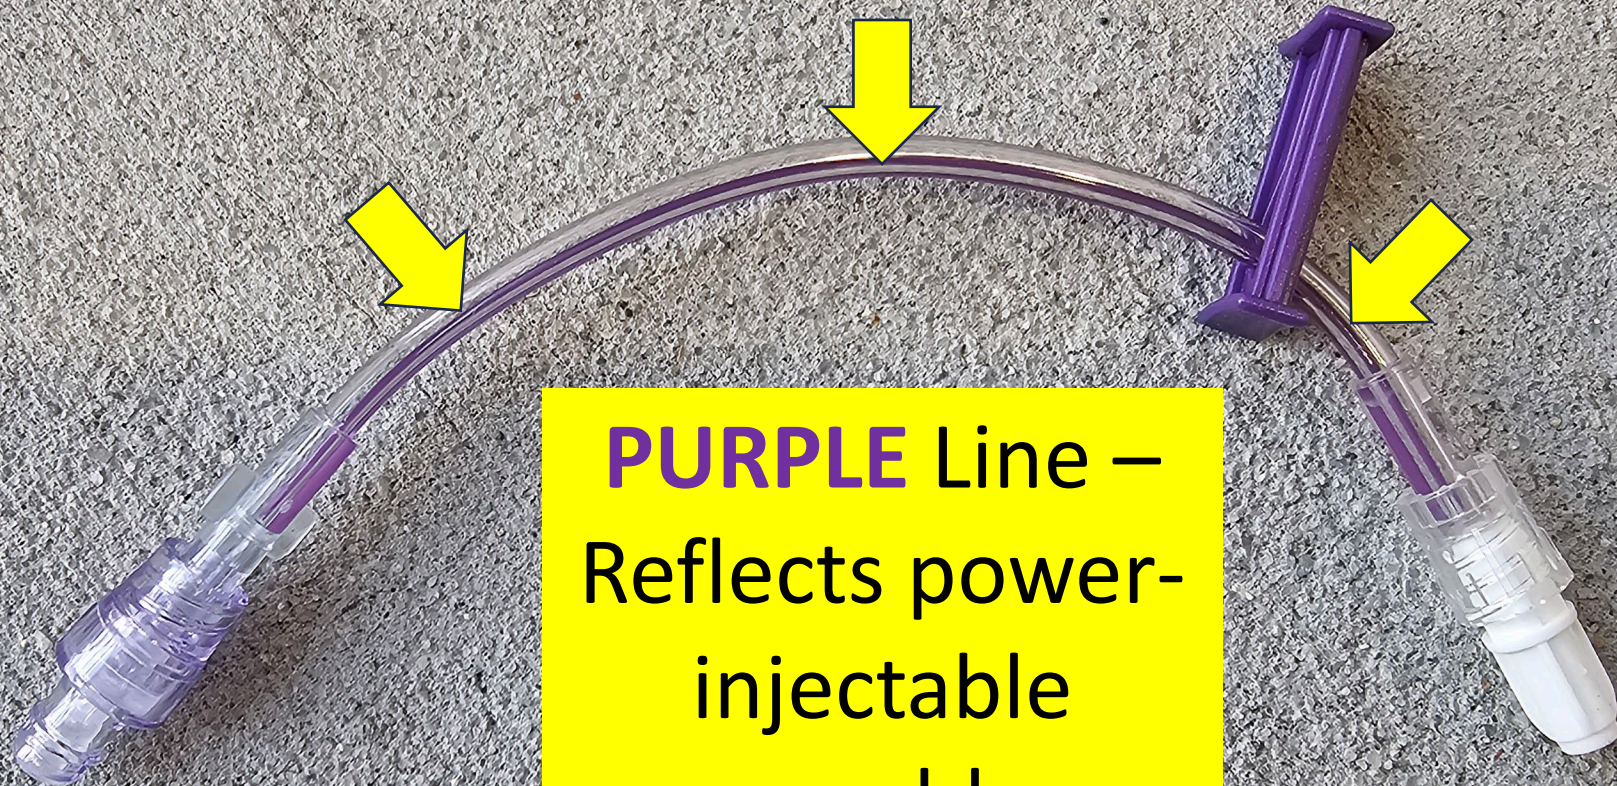

**PURPLE** Line –  
Reflects power-  
injectable  
capable

**NEW**

# - General Overview (cont.)



Expiration  
Date  
Information

A red banner with a white shadow, featuring the word "SUMMARY" in white, bold, uppercase letters. The banner has a slight curve and is set against a white background.

**SUMMARY**

# Kit Individual Item

# Existing Kit

# New Kit

<b>Extension Set with Luer Activated Valve</b>	<b>NON-pressure rated</b> - luer activated valve	<b>Pressure Rated</b> - luer activated valve
<b>Alcohol Pad</b>	2 – medium	2 – large
<b>Gauze</b>	2 – 4” x 4”	2 – 2” x 2” (change in progress to 4” x 4”)
<b>IV Site Dressing</b>	1 – Veni-Gard	1 – Veni-Gard
<b>Tourniquet</b>	1 – Single Use (white)	1 – Single Use (orange)

